




M-0010-9FC

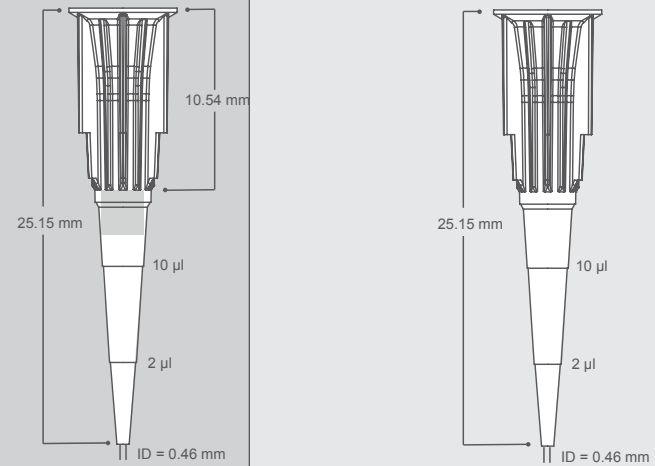

**M-0010-9SC
M-0010-9RC**

Description	10 µl Filter Tip	10 µl Tip	
	M-0010-9FC	M-0010-9SC	M-0010-9RC
Maximum Volume	10 µl	10 µl	
Graduation Marks	Yes	Yes	
Certified Pre-Sterile and Free of Key Contaminants	Yes	Yes	
Material	Clear polypropylene	Clear polypropylene	
Packaging	96 tips per rack, 10 racks per pack, 5 packs per case	96 tips per rack, 10 racks per pack, 5 packs per case	96 tips per card, 20 cards per pack, 5 packs per case, or Tip Eject™
X-Resin™	Yes	Yes	
FlexFit™	Yes	Yes	
Blade™	Yes	Yes	
Delta Filter™	Yes	No	
Technical Drawings			



Quality Testing

RNase/DNase	Products are washed in distilled water and concentrated via centrifugation. Samples are added to previously established nucleic acid standards, incubated for one hour at 37°C, and tested on a 2% gel using electrophoresis. Products must show no degradation of standards to pass. Test sensitivity is 10 ⁻⁷ Kunitz units/μl.
Nucleic Acid	Products are washed in distilled water and concentrated via centrifugation. Then, samples are added to protocol specified PCR reactions and thermal cycled for 50 cycles. A 2% agarose gel electrophoresis is used to examine experimental samples, positive controls, and negative controls. To pass, product samples must show no DNA amplification. Test sensitivity is 10 ng.
Endotoxin/Pyrogen	Products are tested for endotoxins by using the Limulus Amebocyte Lysate (LAL) gel assay according to FDA guidelines. Test sensitivity is 0.06 EU/ml.
Trace Metal	Products are washed in distilled water. The sample is then tested using reflectometry using a single strip test for the following metals: Ca, Cu, Fe, K, Mg, Mn and Ni. Standard solutions are used as positive controls. A reader is used to detect metals to a sensitivity of 500 mg/L.
PCR Inhibitor	Products are tested via PCR amplification and gel electrophoresis analysis. Samples must show normal amplification to be considered free of PCR inhibitors.
Sterilization	Products are sterilized using electron beam irradiation.
CV Test	Each lot of Biotix product is CV tested and the resulting CV is then printed on the pack label. The volume tested is equal to the maximum volume per tip size.
TIR-Total Indicated Runout	Biotix pipette tips are tested to ensure that they meet the SBS standards. Individual products specify their compatibility with 96, 384 or 1536-well plates.

Proprietary Technologies

FlexFit™	Ergo design Patents Pending
X-Resin™	Proprietary resin, virgin polypropylene
Chem-Resin™	Neutral surface tension for working with polar solvents and electronegative reagents. Biologically inert with no contaminating extractables.
Delta Filter™	Color change filter Patents Pending
Blade™	Minimal distal end orifice Patents Pending

Pipettor Compatibility:

Biohit Proline™ 10 μl
 Brand Transferpette S™ 10 μl
 Capp™ 10 μl
 CLP Beta-Pette™ 2 μl and 10 ul
 CLP Poseidon™ 2 μl and 10 ul
 CLP Poseidon Electronic™ 20 μl
 Eppendorf Reference™ 2.5 μl
(works with M-0010-9SC)
 Eppendorf Reference™ 10 μl

Eppendorf Research™ 2.5 μl
(works with M-0010-9SC)
 Eppendorf Research™ 10 μl
 Eppendorf Research Plus™ 2.5 μl
(works with M-0010-9SC)
 Eppendorf Research Plus™ 10 μl
 Eppendorf Xplorer™ 10 μl
 Finnpiquette™ 10 μl and 50 μl
 Finnpiquette™ Electronic 10 μl

Finnpiquette F1™ 10 μl
 Gilson Pipetman™ P2 and P10
 Hamilton™ 2 μl and 10 μl
 Nichiryo Nichipet EX™ 10 μl
 Nichiryo Oxford Benchmate™ 2 μl
 Nichiryo Oxford Multimate™ 10 μl
 Socorex Calibri 822™ 10 μl
 VWR Ultra High Performance™
 2 μl and 10 μl

©2014, Biotix, Inc. All rights reserved

Biotix, Fluid Innovation, Delta Filter, X-Resin, Chem-Resin, Blade, FlexFit, Statix, Leave Nothing Behind, BioReady, Tip Eject, and XTreme Quality are registered trademarks or trademarks of Biotix, Inc. All other brands and names contained herein are the property of their respective owners.